




Page 1 of 9

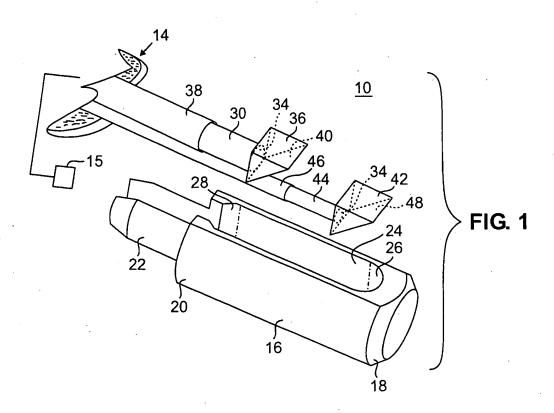

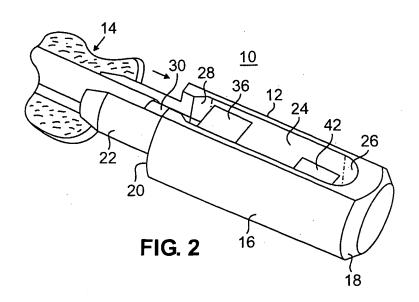




APR 2 3 2004

Page 2 of 9

Appln No.: 10/037,306 Applicant(s): Simon M. Furnish MULTI-FIBER CATHETER FOR VP DETECTION

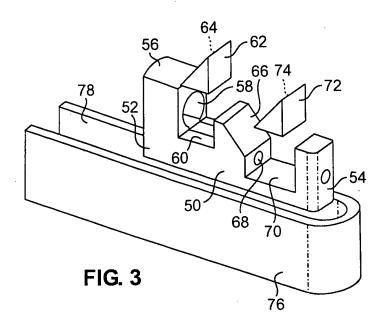



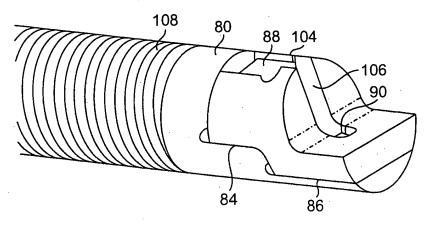


FIG. 4(a)




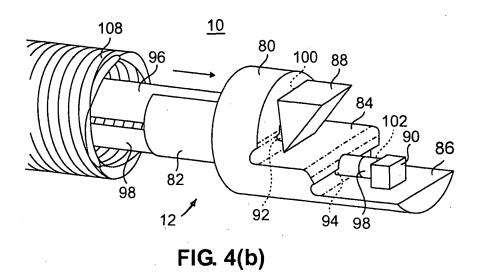


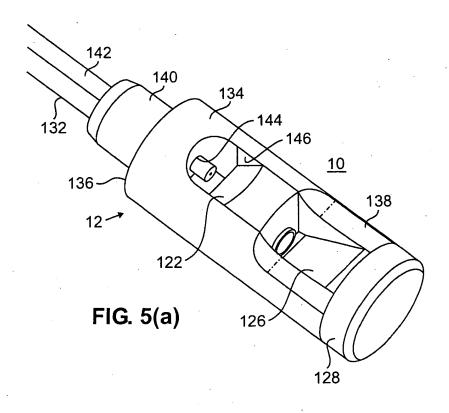

Page 4 of 9

Appln No.: 10/037,306 Applicant(s): Simon M. Furnish MULTI-FIBER CATHETER FOR VP DETECTION

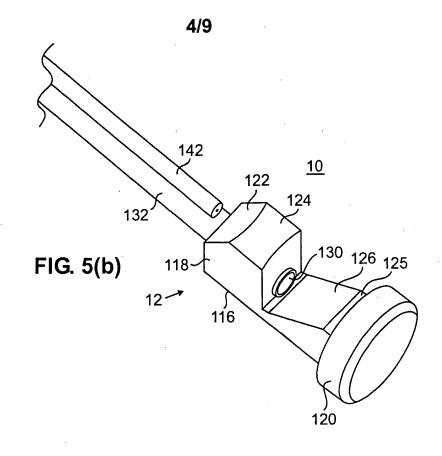

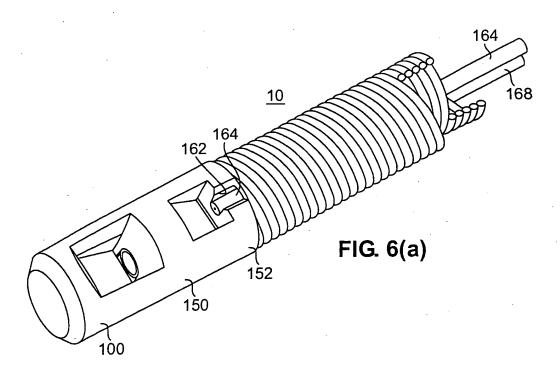




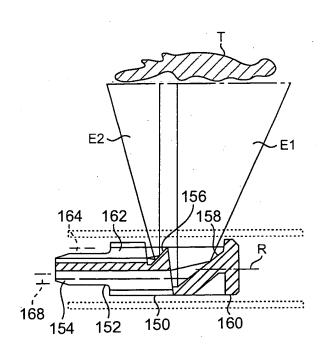



FIG. 6(b)

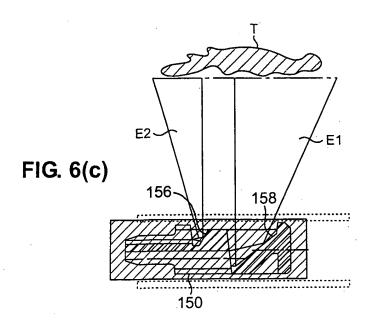


6/9

Page 6 of 9



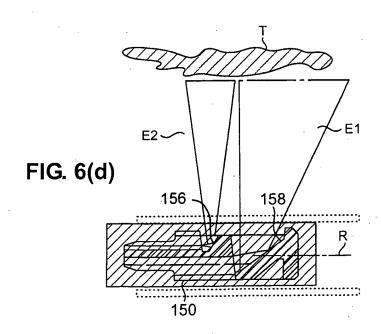



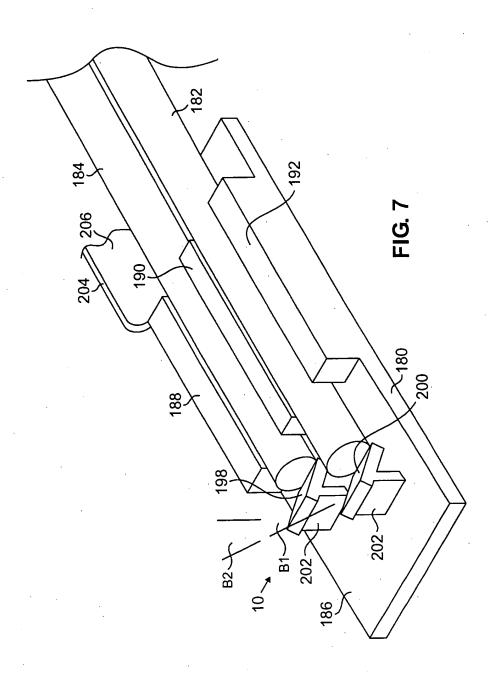



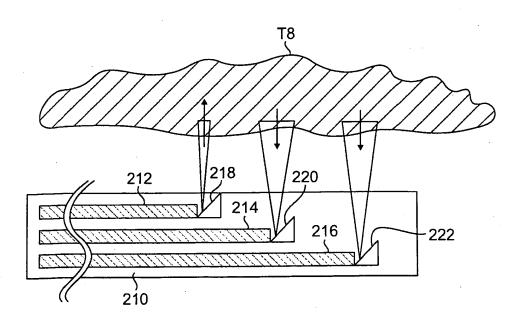


FIG. 8

9/9

Page 9 of 9

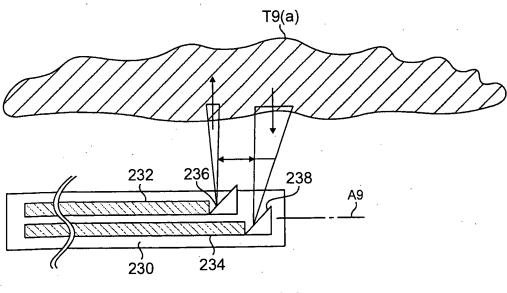


FIG. 9(a)

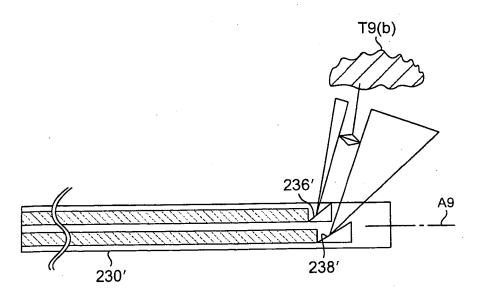


FIG. 9(b)